


# Chromatogram

Sample Name :                      Sample #: 013                      Page 1 of 1  
FileName : C:\Data\data013-20100208-130235.raw  
Date : 2/8/2010 1:03:19 PM  
Method : X-C-2.mth                      Time of Injection: 2/8/2010 1:02:28 PM  
Start Time : 0.00 min                      End Time : 0.70 min                      Low Point : -46.56 mV                      High Point : 993.63 mV  
Scale Factor: 1.0                      Plot Offset: -46.56 mV                      Plot Scale: 1040.2 mV

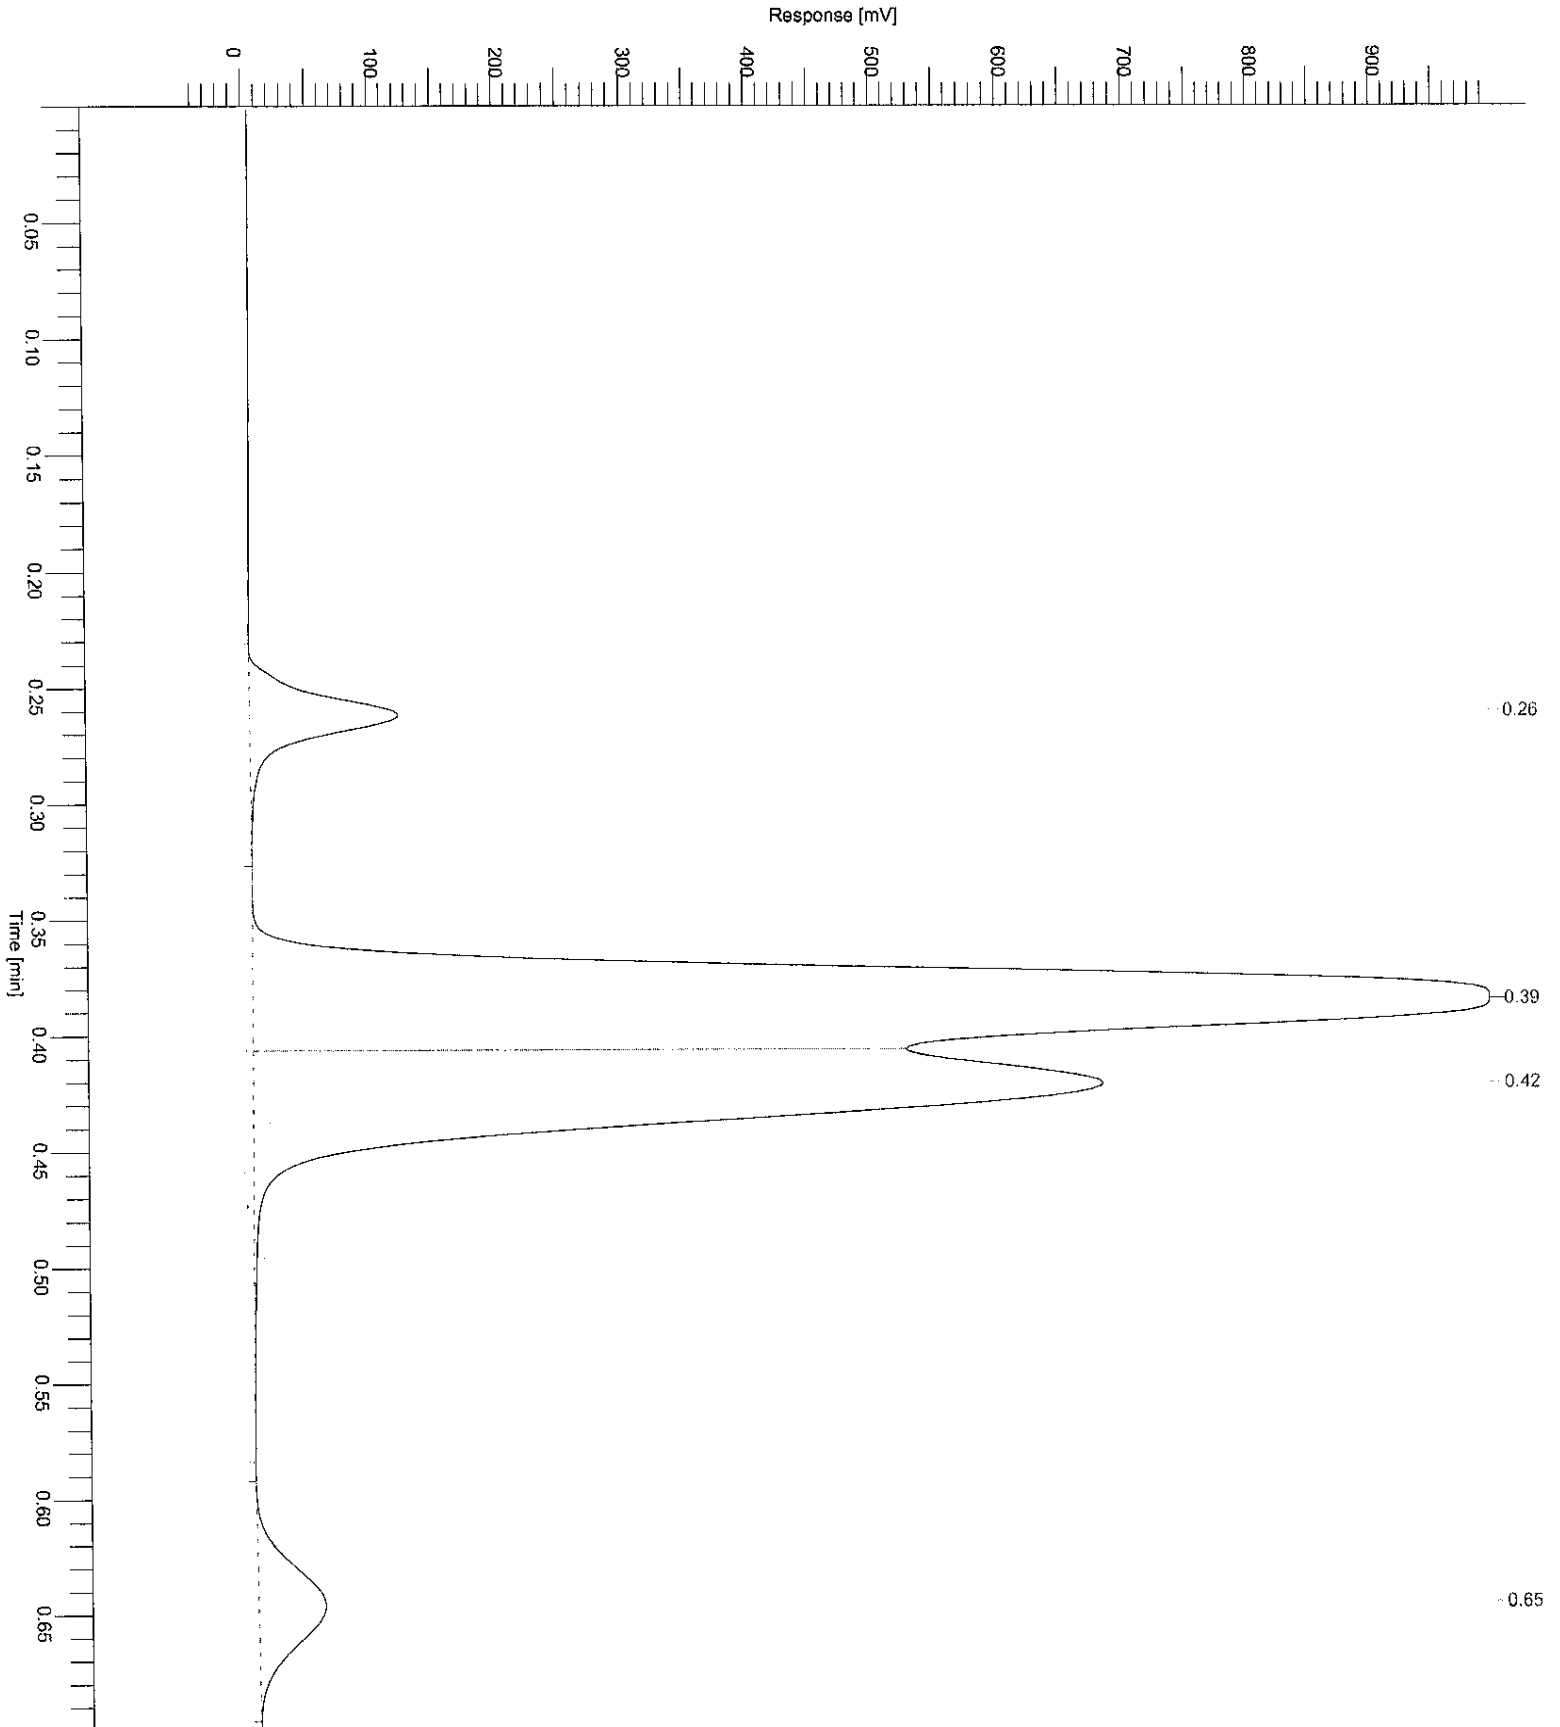

Software Version : 6.1.2.0.1:D19  
 Operator : user02  
 Sample Number : 013  
 AutoSampler : NONE  
 Instrument Name : Autosystem XL  
 Instrument Serial # : None  
 Delay Time : 0.00 min  
 Sampling Rate : 12.5000 pts/s  
 Volume Injected : 1.000000 ul  
 Sample Amount : 1.0000  
 Data Acquisition Time : 2/8/2010 1:02:28 PM

Date : 2/8/2010 1:03:18 PM  
 Sample Name :  
 Study :  
 Rack/Vial : 0/0  
 Channel : A  
 A/D mV Range : 1000  
 End Time : 0.70 min

Area Reject : 0.000000  
 Dilution Factor : 1.00  
 Cycle : 13

Raw Data File : C:\Data\data013-20100208-130235.raw

Result File : C:\Data\data013-20100208-130317.rst

Inst Method : C:\Methods\X-C-2 from C:\Data\data013-20100208-130317.rst

Proc Method : C:\Methods\X-C-2

Calib Method : C:\Methods\X-C-2

Sequence File : C:\Sequences\Lab X-C try 2.seq

## DEFAULT REPORT

Peak #	Time [min]	Area [ $\mu\text{V}\cdot\text{s}$ ]	Height [ $\mu\text{V}$ ]	Area [%]	Norm. Area [%]	BL	Area/Height [s]
1	0.261	142414.64	118126.08	4.18	4.18	BB	1.2056
2	0.385	1876742.91	989763.90	55.10	55.10	BV	1.8962
3	0.421	1261306.31	678210.22	37.03	37.03	VB	1.8598
4	0.645	125333.51	53436.80	3.68	3.68	BB	2.3455
		3405797.37	1.84e+06	100.00	100.00		

### Missing Component Report

Component Expected Retention (Calibration File)

All components were found